



### Kind of Test

**Test Equipment**

Test Equipment	Flow Analyzer PF 300
Serial Number	BA101233
Calibration Date	12.12.2006

**Test Object**

Customer	Hospital Name
Department	Departement
Brand Name	Ventilator Name
Type	Type
Serial Number	00000
Operating Hours	0 h

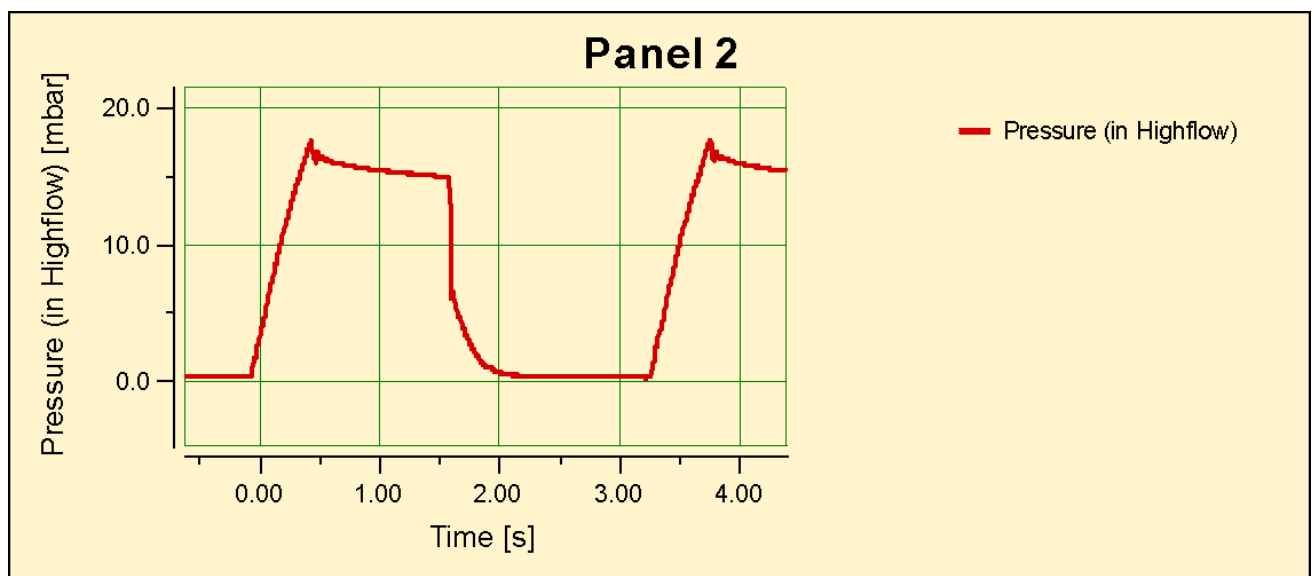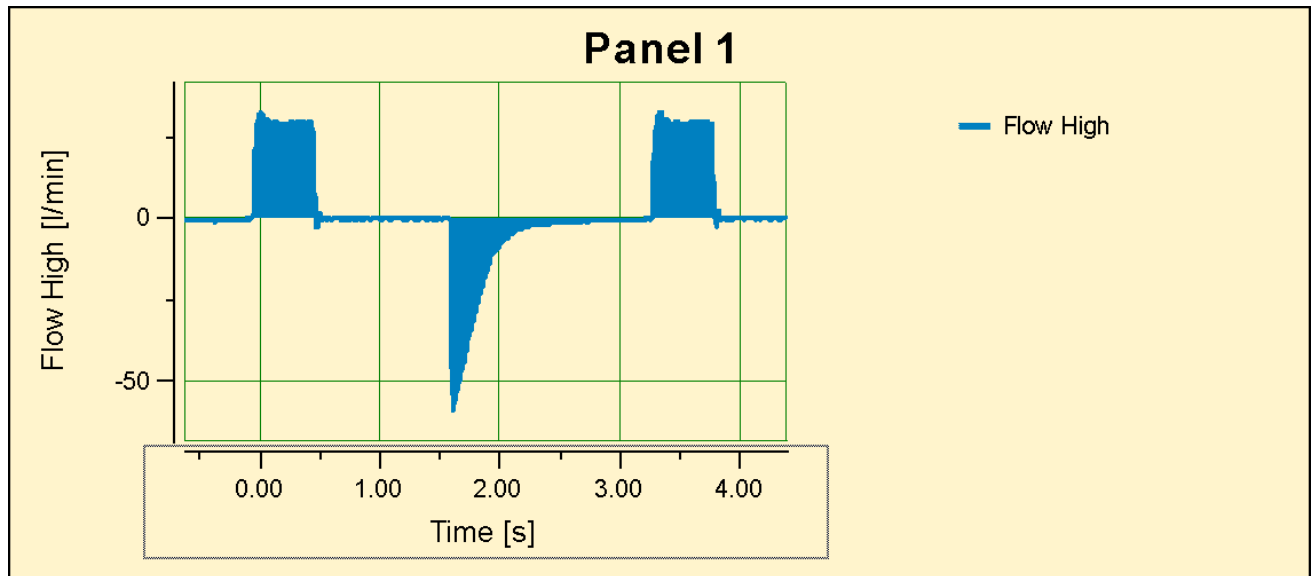

Measuring values	Unit	Value	Min	Max	Average	Setpoint	Limit Lo	Limit Hi	OK
Flow High	l/min	0.0	-106.4	117.6	0.1				
Pressure Difference	mbar	0.00	-0.09	0.16	0.05				
Pressure High	bar	0.000	-0.003	0.002	-0.001				
Pressure Atmospheric	mbar	974	974	974	965	974	970	980	✓
Oxygen	%	19.8	19.7	20.1	20.0	21	18	23	✓
Temperature	°C	27.3	26.1	27.9	27.3	27	20	30	✓
Humidity	%	18	16	21	19	19	15	25	✓
Dew Point Temperature	°C	0.9	-0.8	3.4	1.2	1.4	0.2	2	✓

Respiratory Parameters	Unit	Value	Min	Max	Average	Setpoint	Limit Lo	Limit Hi	OK
Rate	b/min	18	2.6	18.1	17.1	18	16	20	✓
I : E	---	1:1.0	1:16.4	4.9:1	1:1.1	1:1.0	1:1.5	1:0.5	✓
Ti	s	1.65	1.34	10.61	1.70	1.65	1.4	1.7	✓
Ppeak	mbar	17.9	17.3	80.9	28.7	18	16	20	✓
PEEP	mbar	0.3	0.0	5.1	0.4	0.5	0	1	✓
Vte	ml	235	71	523	237	250	230	270	✓
Vti	ml	251	98	1618	243	250	230	270	✓
Vi	l/min	4.5	1.7	7.4	4.1	4.4	4	5	✓
Pplateau	mbar	15.3	13.2	50.5	16.9	15	13	17	✓
Cstat	ml/mbar	16.7	5.2	54.8	15.7	16	15	17	✓

Comments

---



---



---

Date 12.03.2007

Operator/Tester Name of Tester

Signature

---